
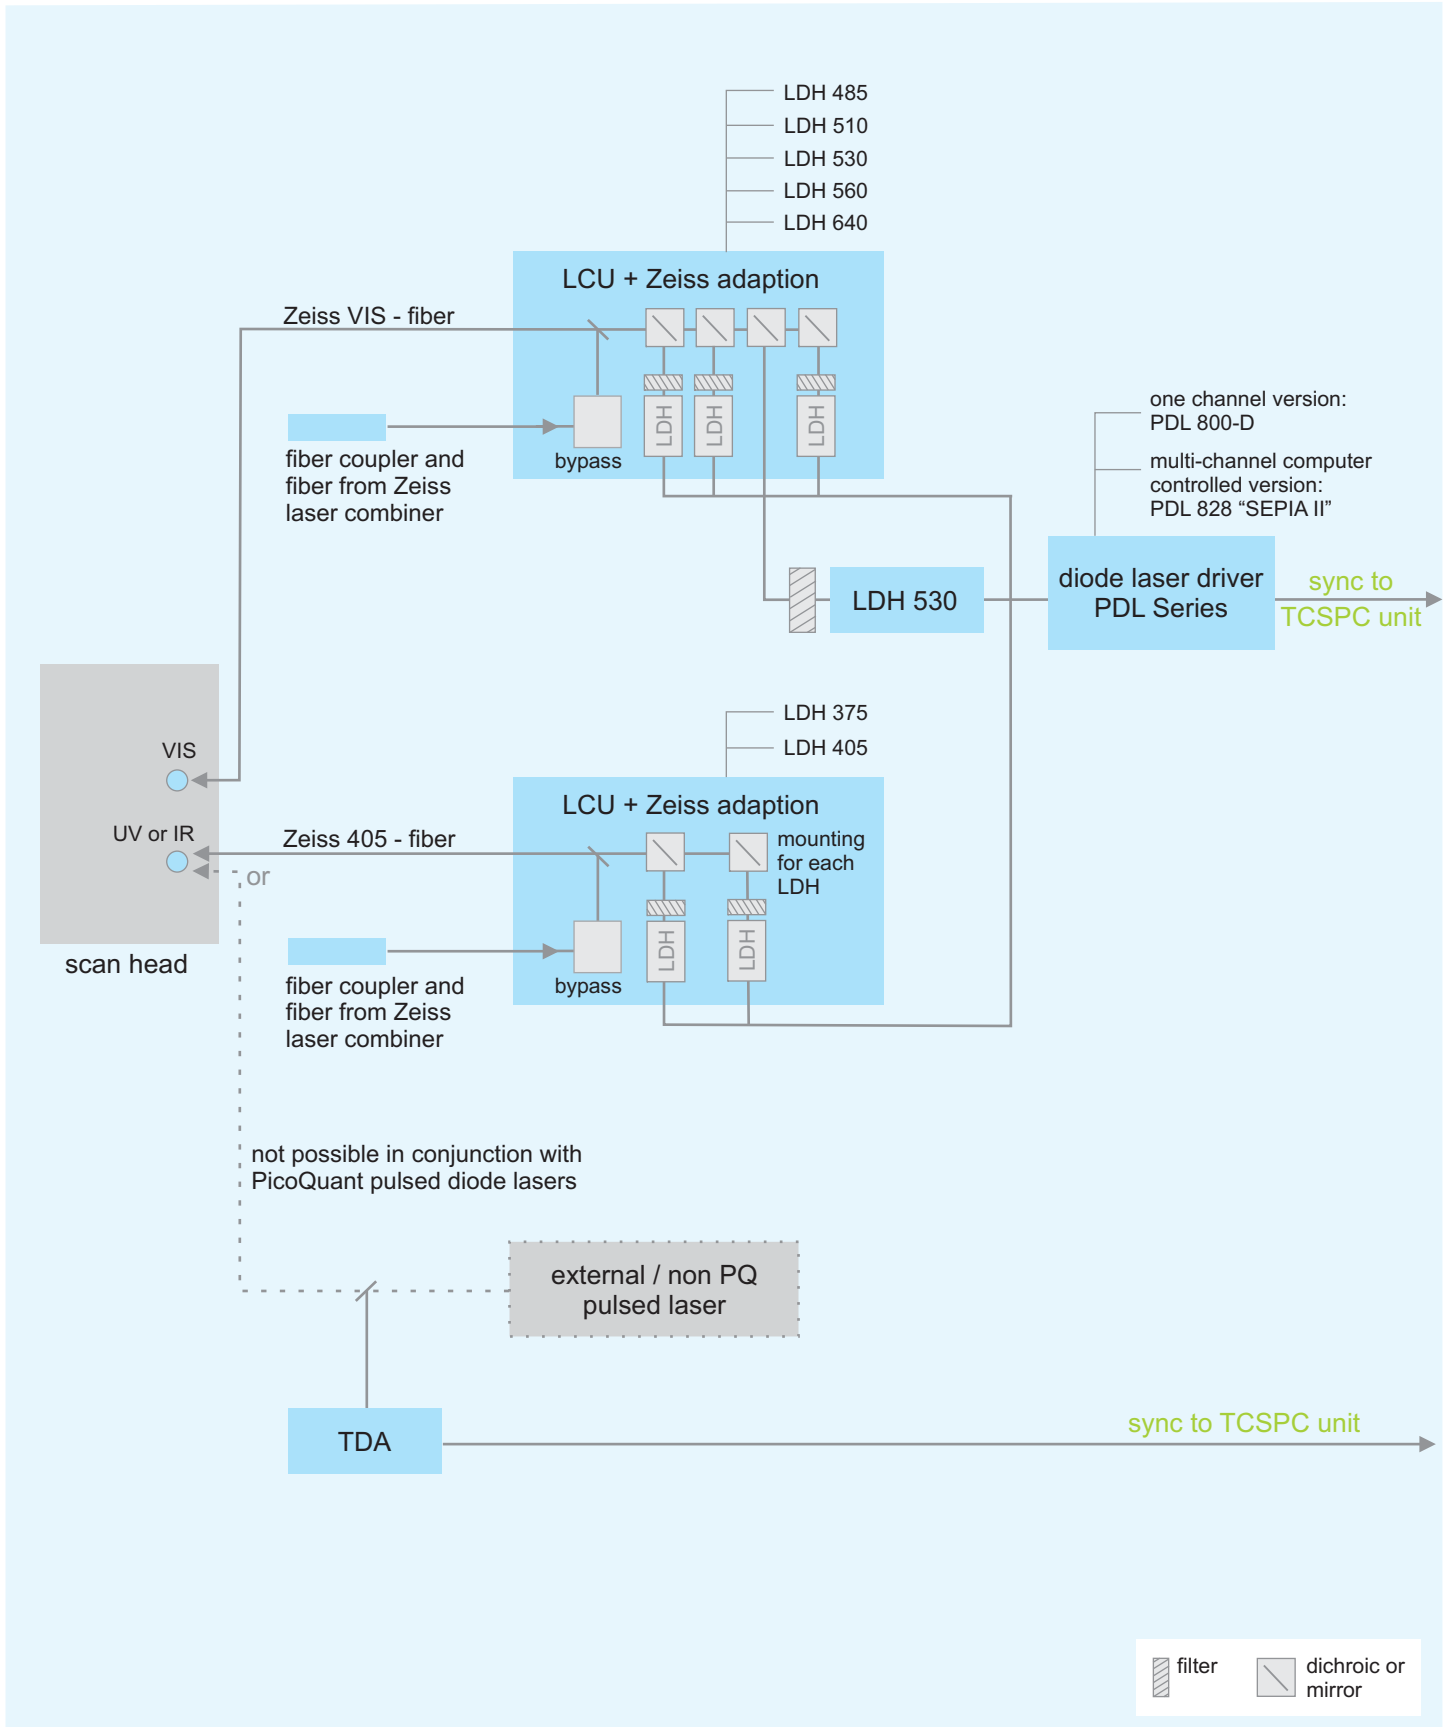



# Excitation Components

## Zeiss LSM 510

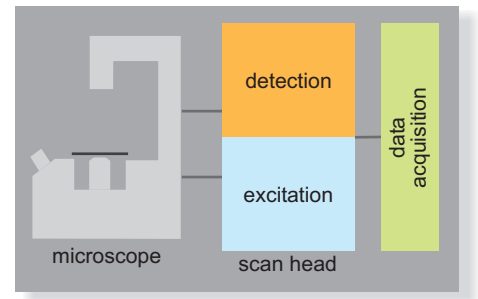


# PMA Detection Components

## Zeiss LSM 510

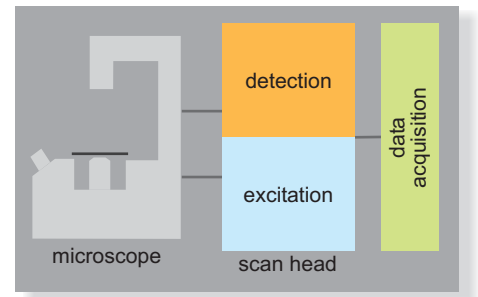

### NDD (Non-descanned Detection)

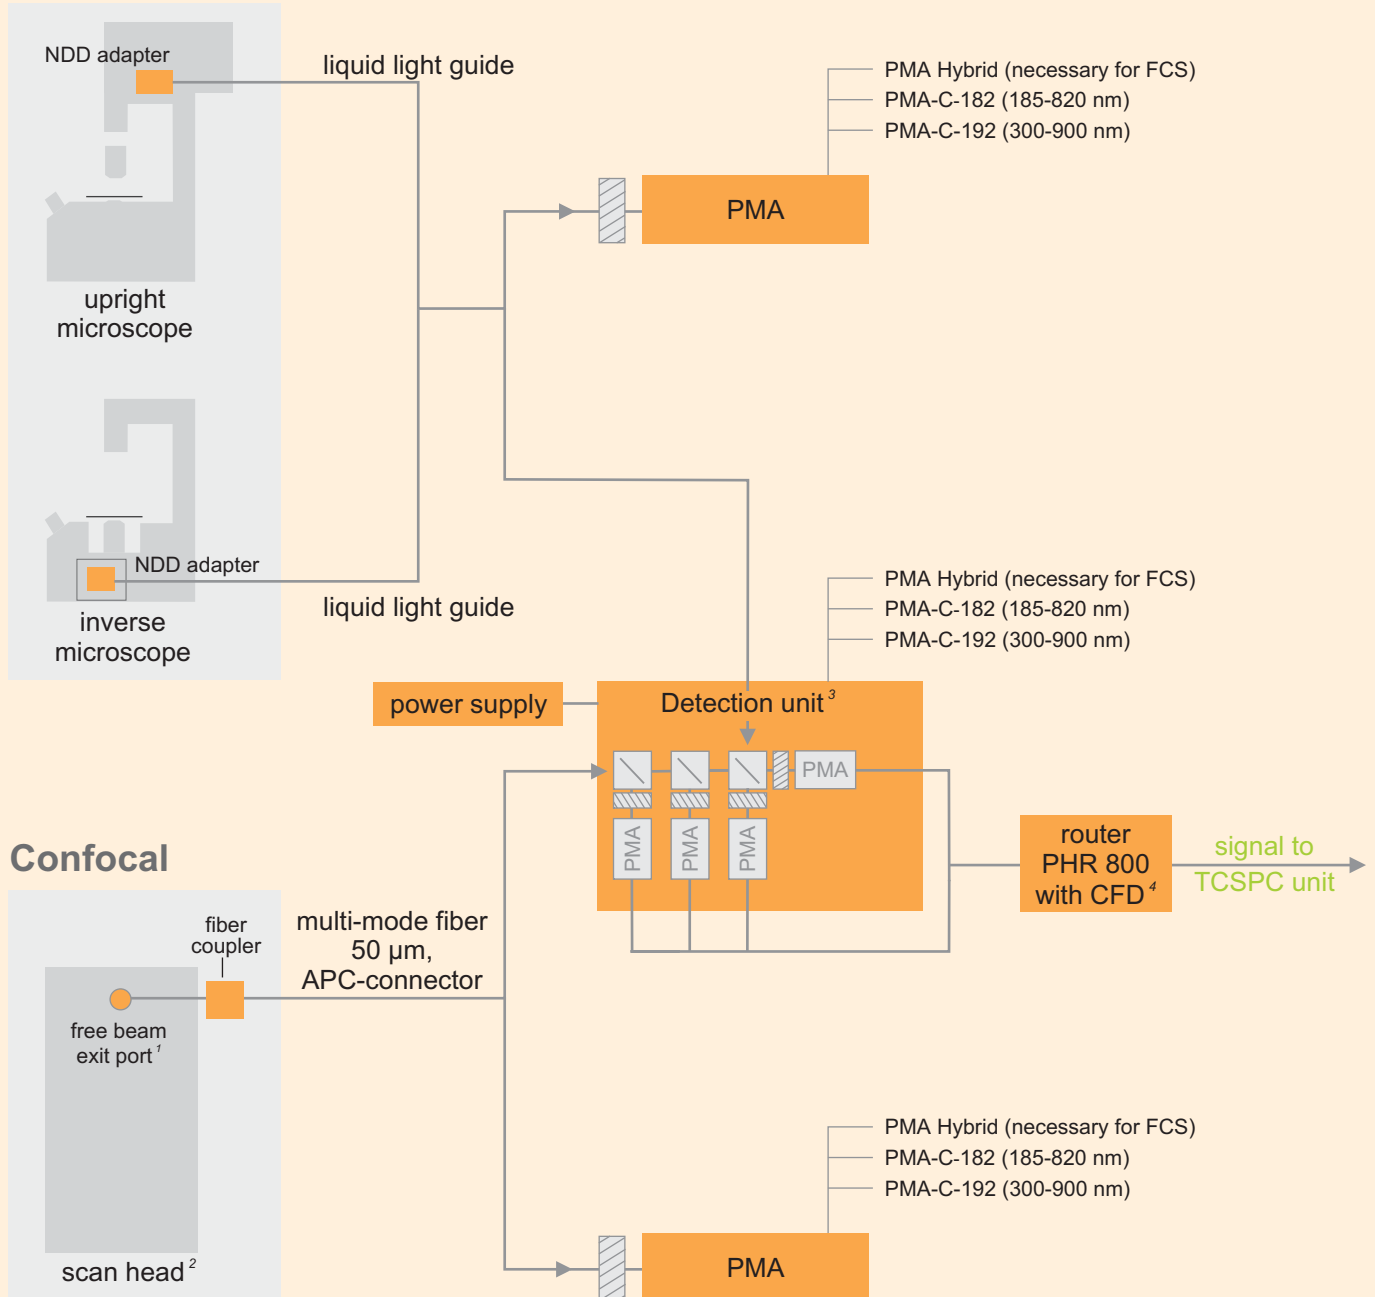

1) LSM must be equipped with a free space exit port. The LSM must be based on an inverse microscope with the LSM at the siteport. It must be placed on an optical table for mounting of the exit port. Combination with Zeiss Confocor requires special "Zeiss splitter".



2) Anisotropy measurements are possible with special two fiber adapter.

3) Detection unit is available with up to four detectors, NDD only with up to 2 detectors possible.

4) Not needed with HydraHarp 400 and TimeHarp 260.



# SPAD Detection Components Zeiss LSM 510

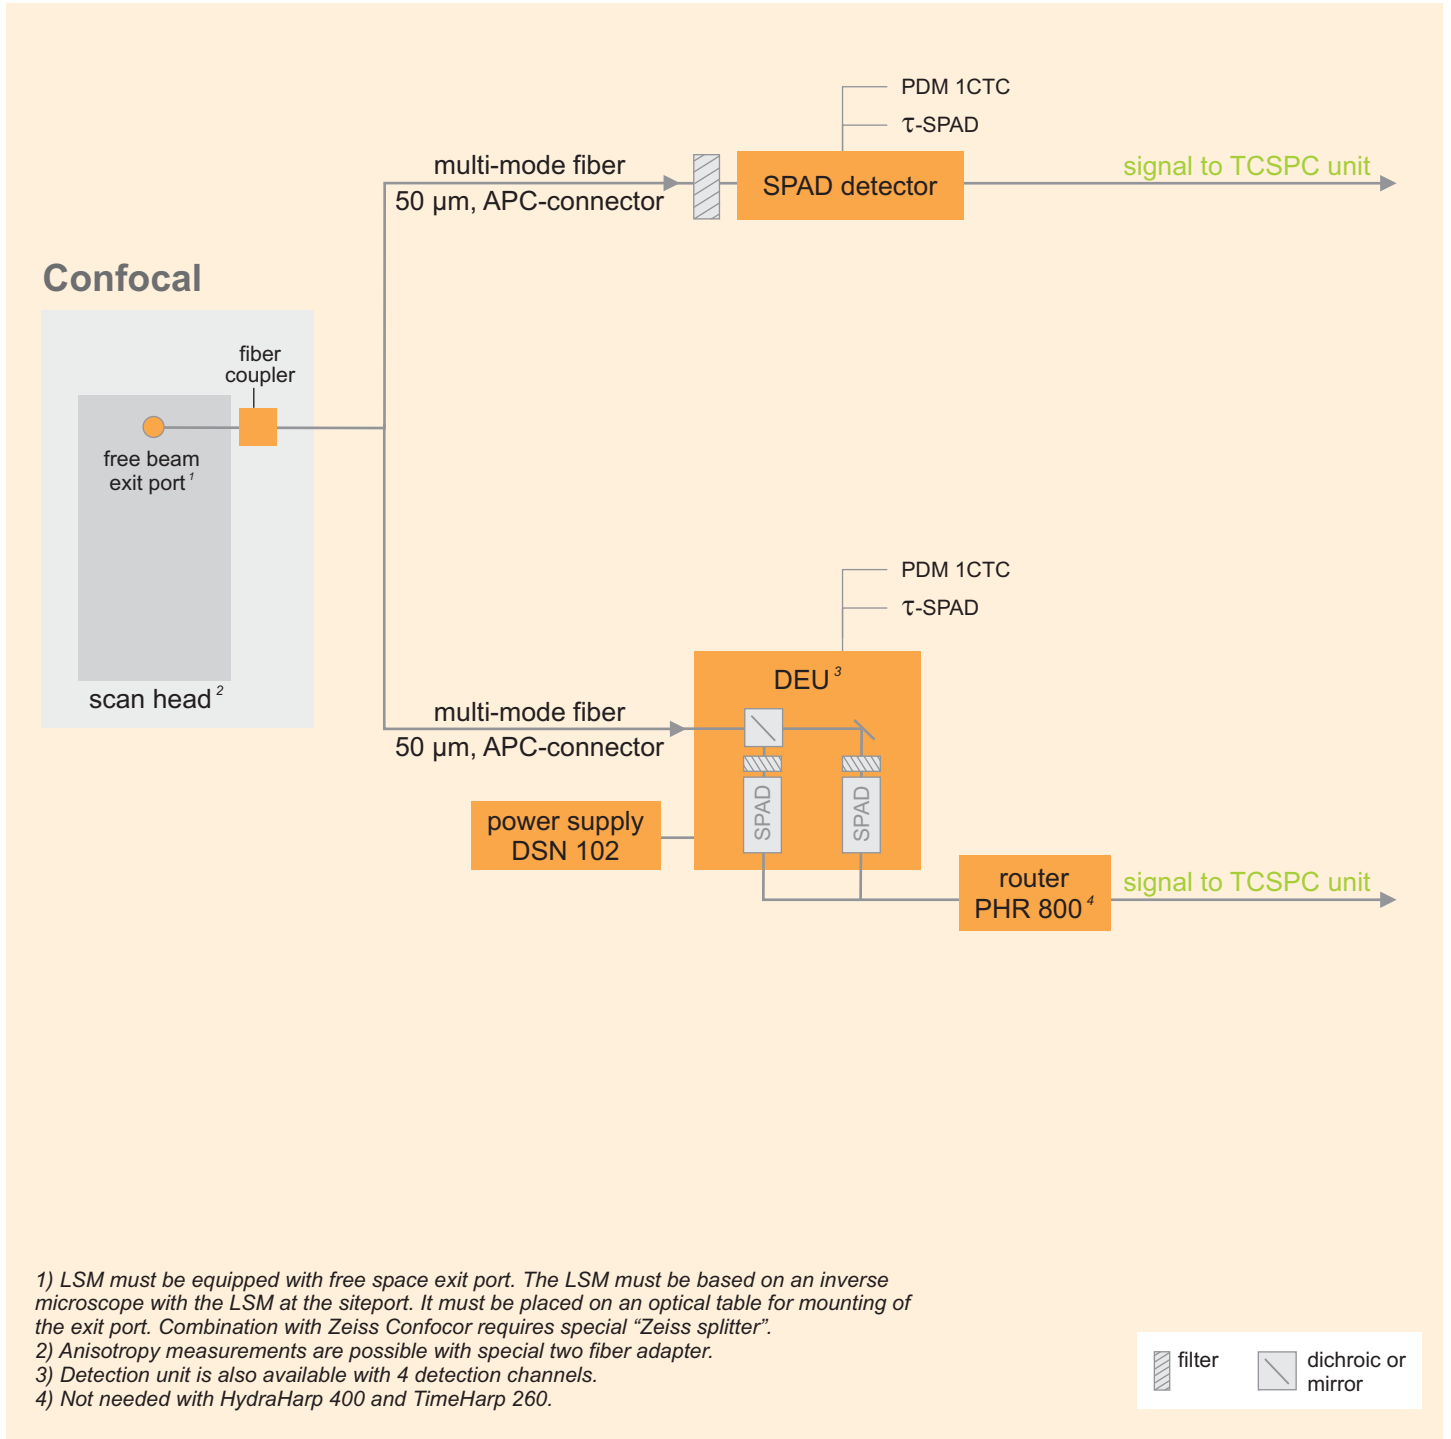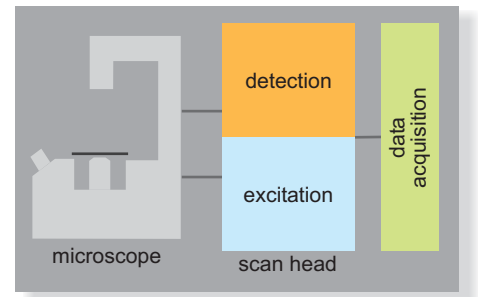



1) LSM must be equipped with free space exit port. The LSM must be based on an inverse microscope with the LSM at the siteport. It must be placed on an optical table for mounting of the exit port. Combination with Zeiss Confocor requires special "Zeiss splitter".

2) Anisotropy measurements are possible with special two fiber adapter.

3) Detection unit is also available with 4 detection channels.

4) Not needed with HydraHarp 400 and TimeHarp 260.

# Components - Data Acquisition Zeiss LSM 510

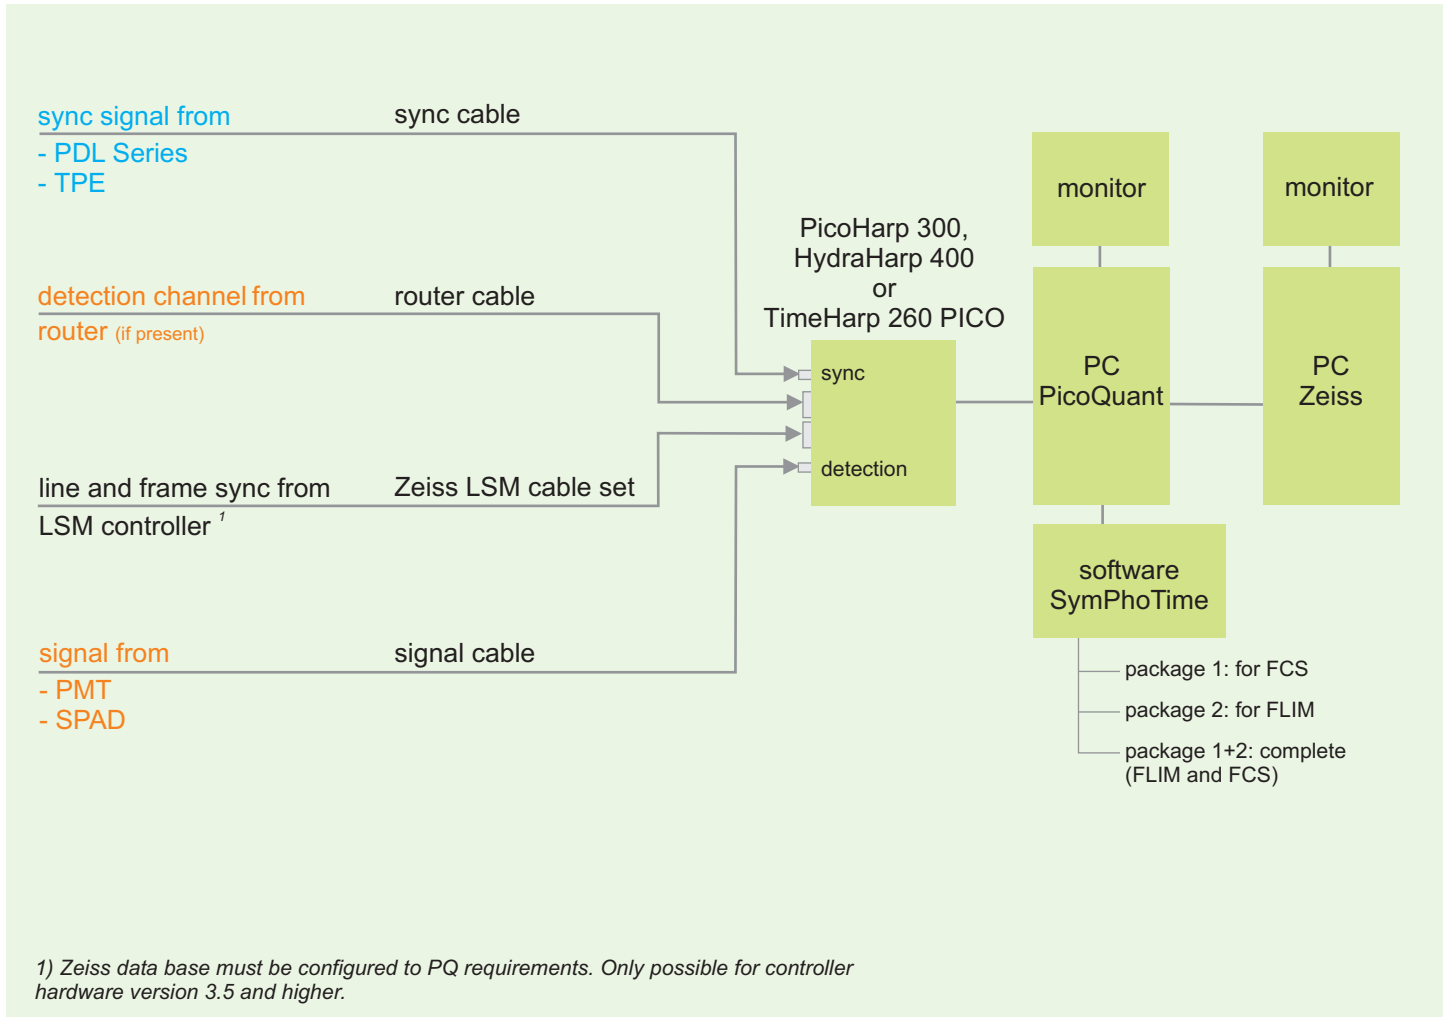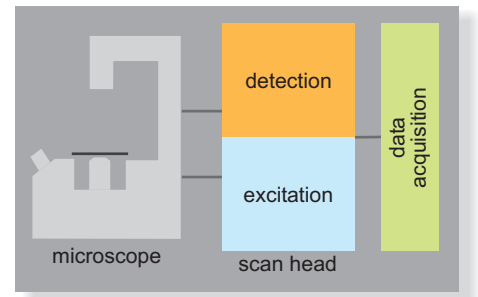

All Information given here is reliable to our best knowledge. However, no responsibility is assumed for possible inaccuracies or omissions. Specifications and external appearances are subject to change without notice. Trademarks or corporate names are used for explanation and identification, to the owner's benefit and without intent to infringe.

© PicoQuant GmbH, June 2015



PicoQuant GmbH  
Rudower Chaussee 29 (IGZ)  
12489 Berlin  
Germany

Phone +49-(0)30-6392-6929  
Telefax +49-(0)30-6392-6561  
Email info@picoquant.com  
WWW <http://www.picoquant.com>