

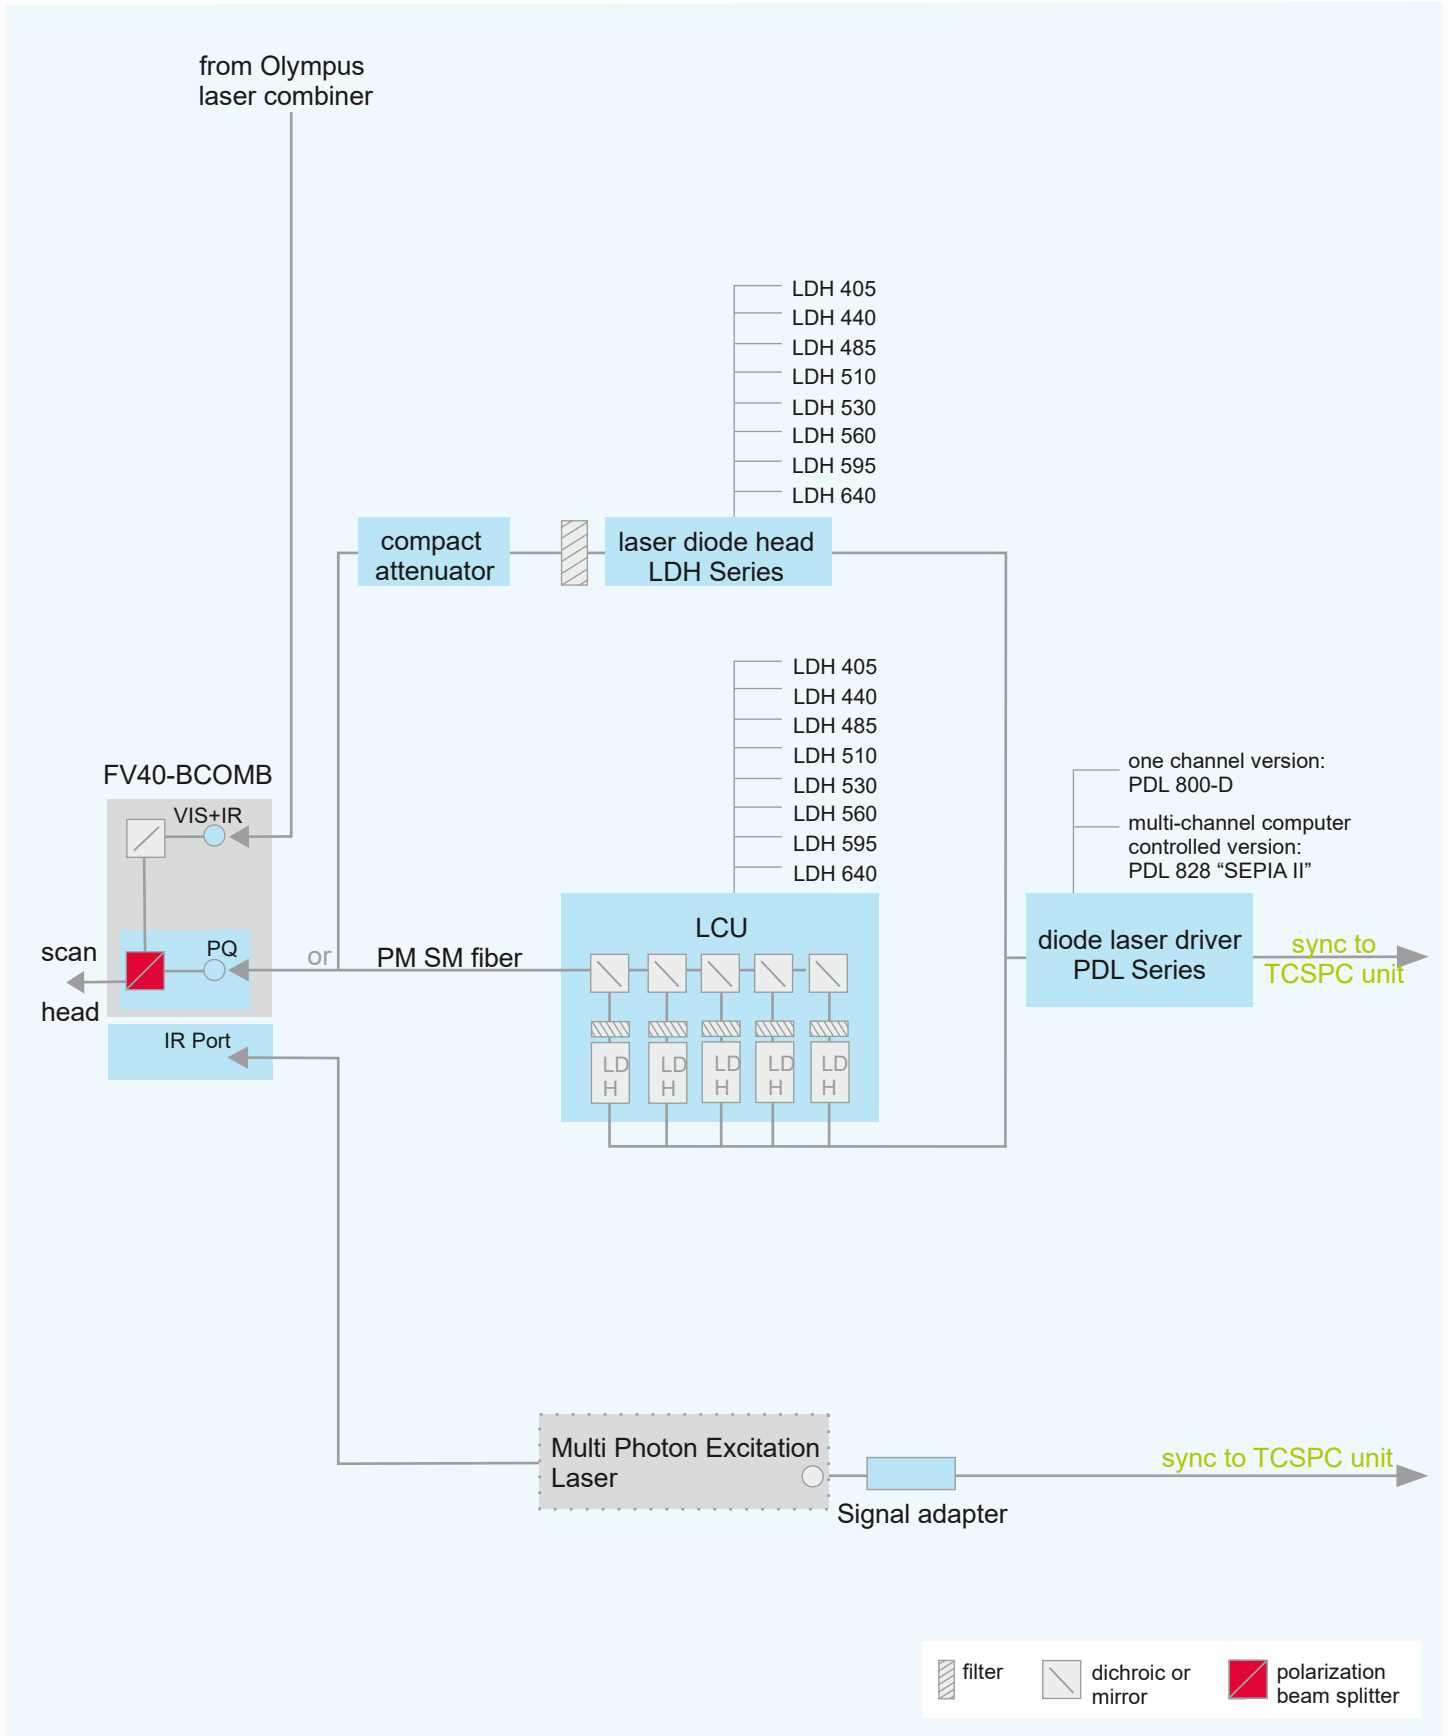
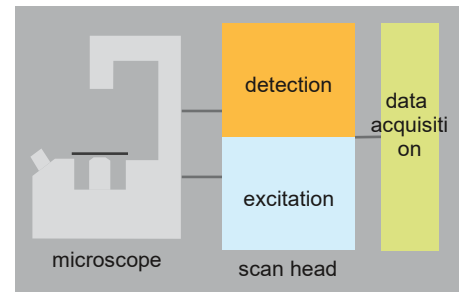


Excitation Components Evident FV5000(MP)

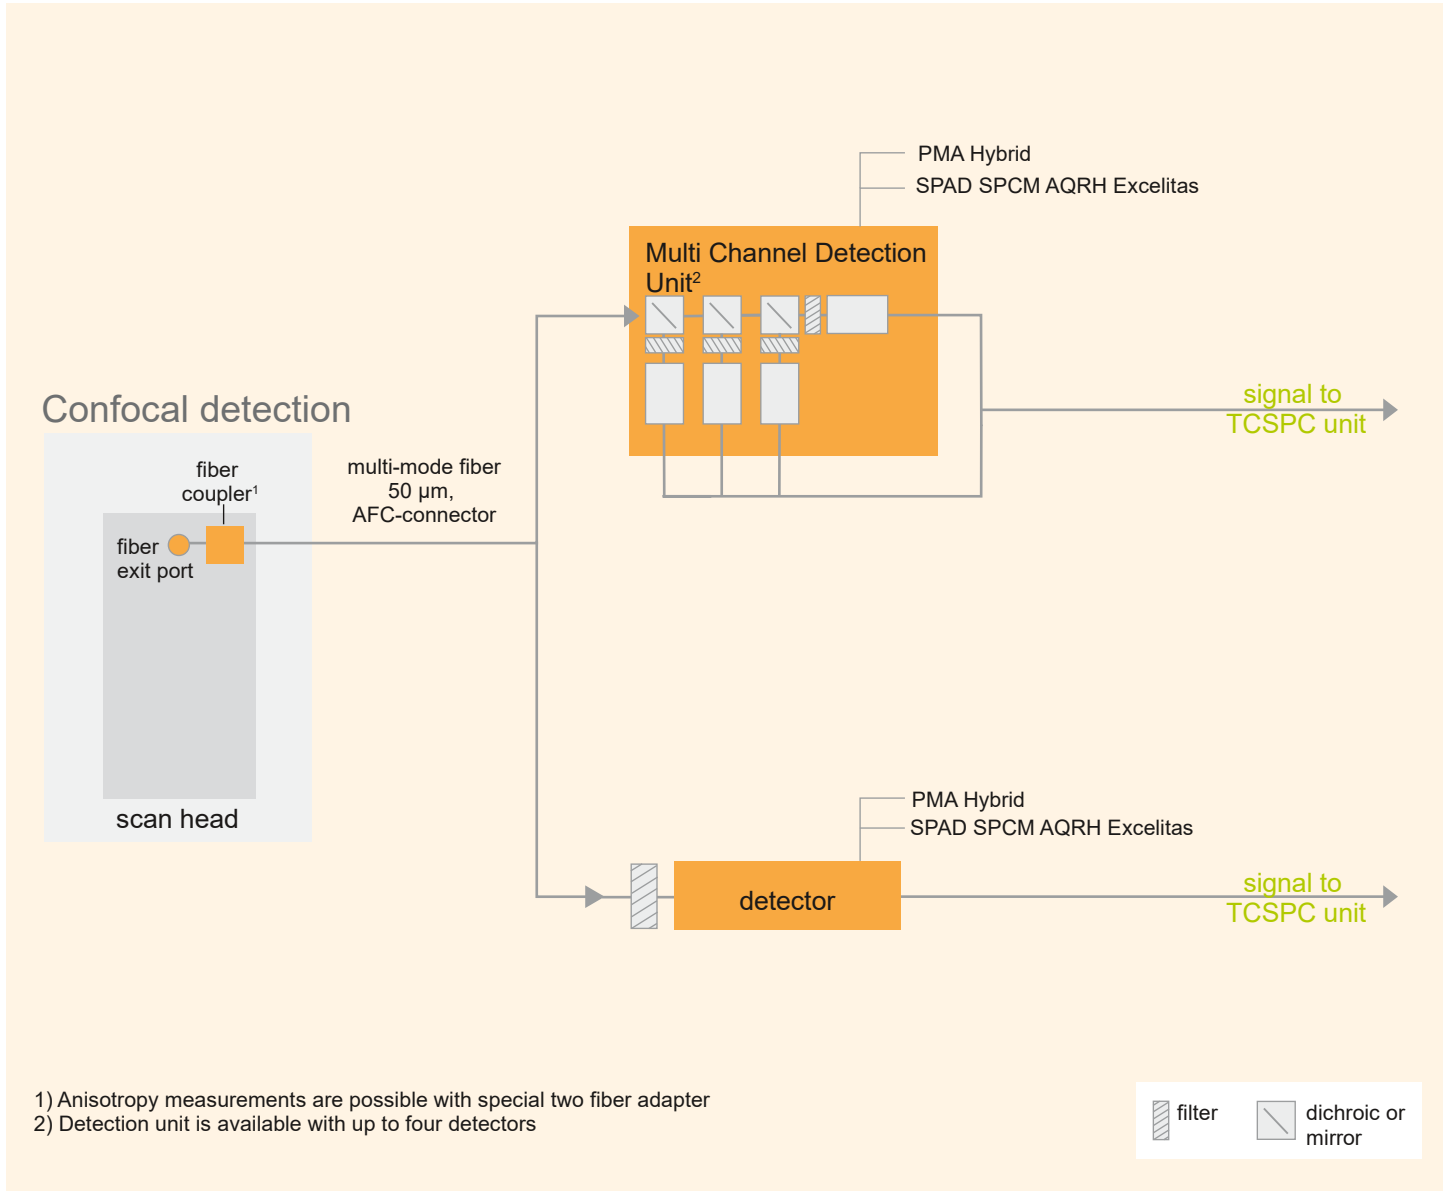


Detection Components

Evident FV5000(MP)

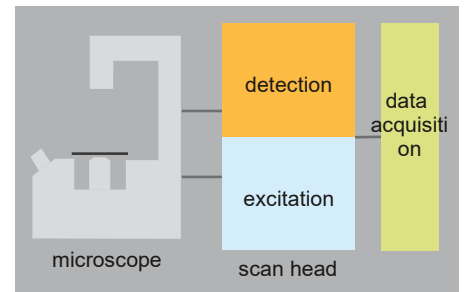


PMA Detection Components

Olympus FV5000MP

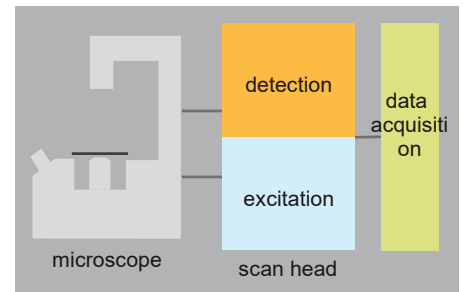

NDD (Non-descanned Detection)


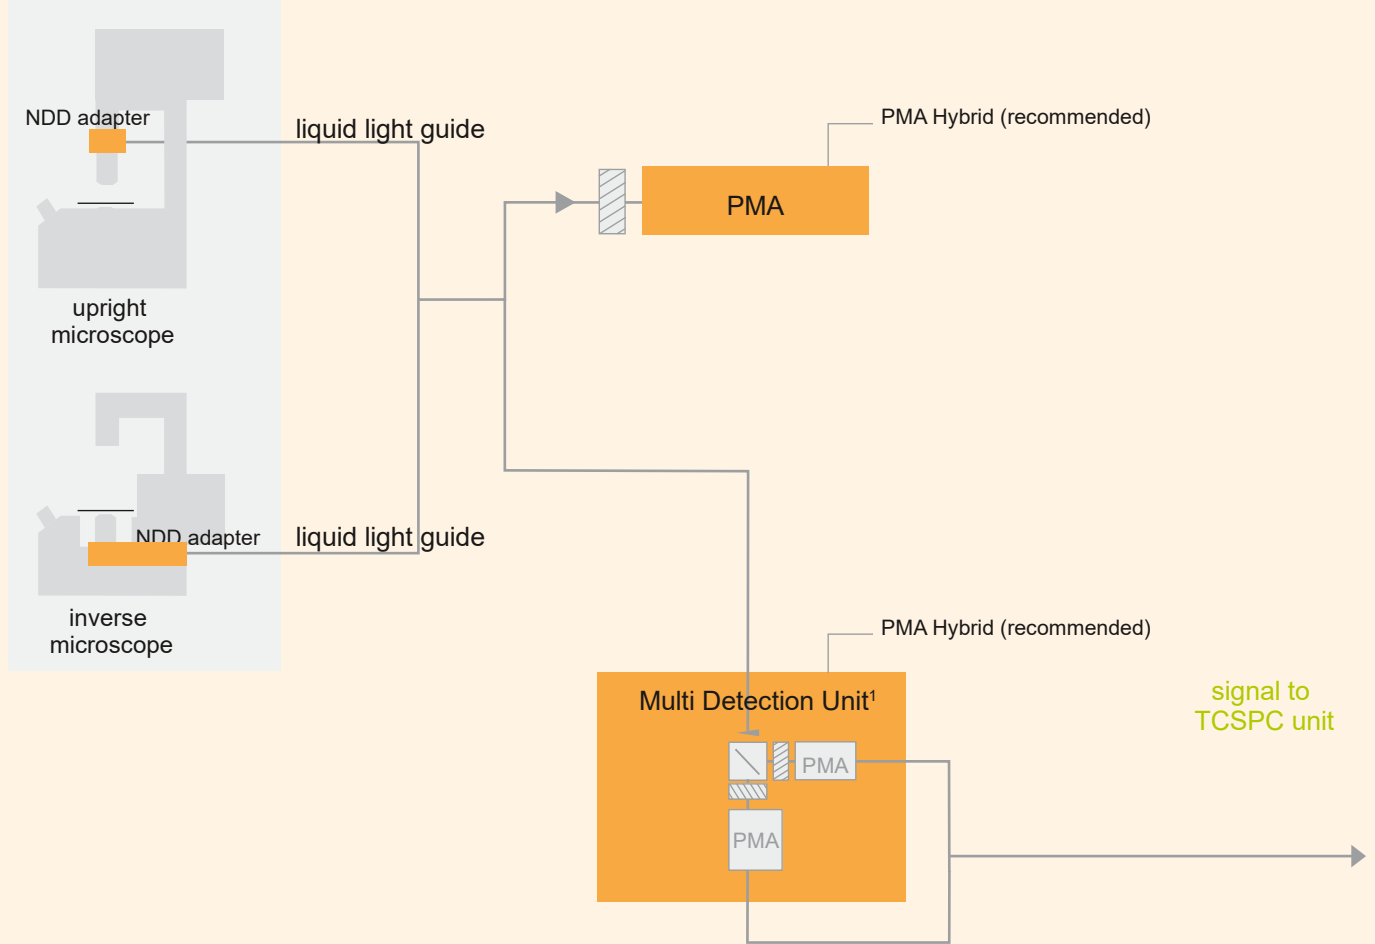


1) Detection unit is available with up to two detectors

- 1) Anisotropy measurements are not possible
- 2) Detection unit is available with up to four detectors, NDD only with up to 2 detectors possible.
- 3) Not needed with MultiHarp150 and TimeHarp 260.



Components - Data Acquisition Evident FV5000(MP)

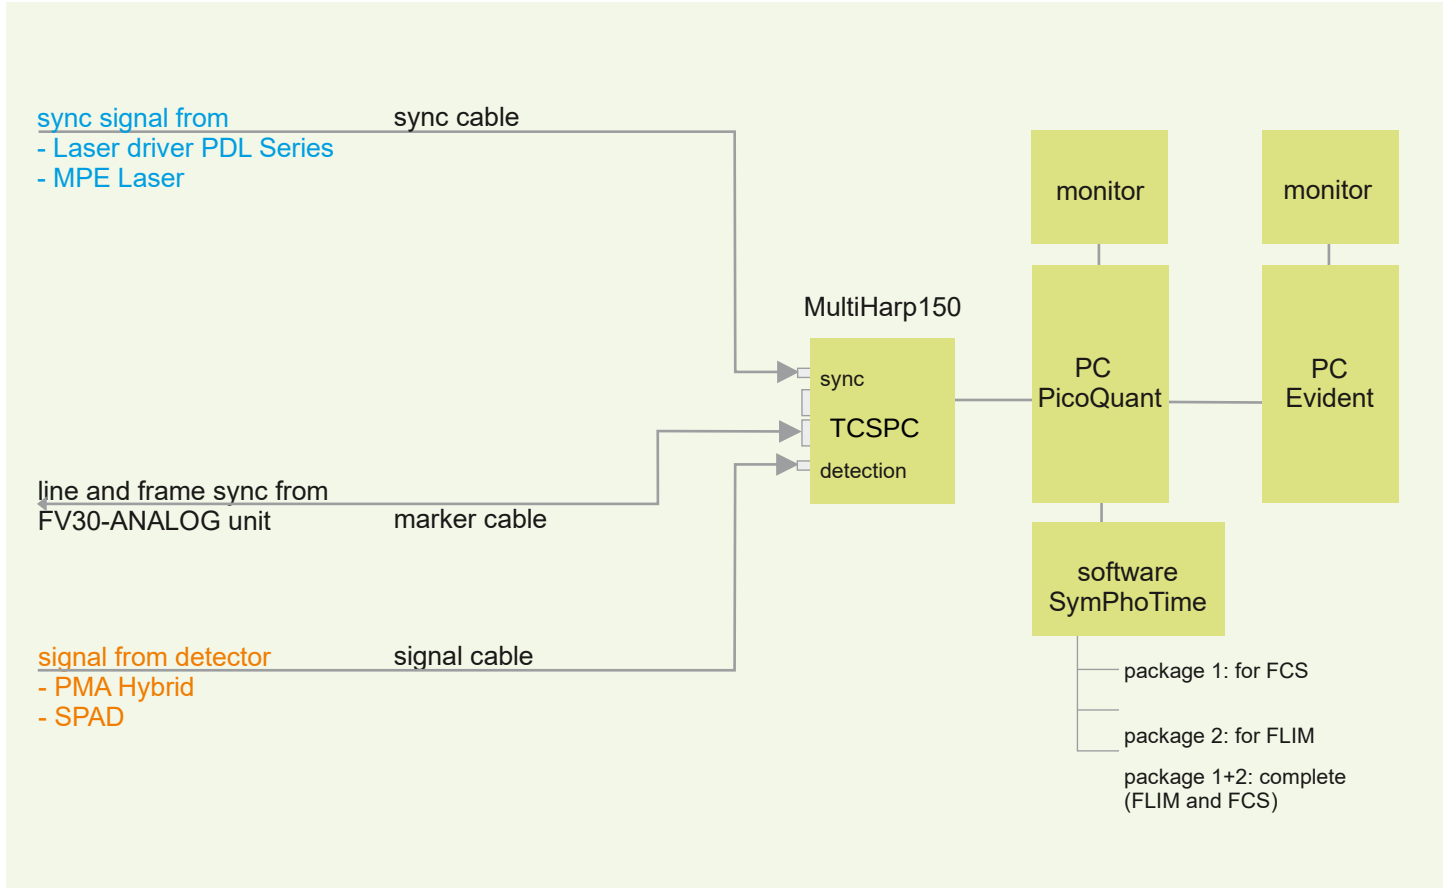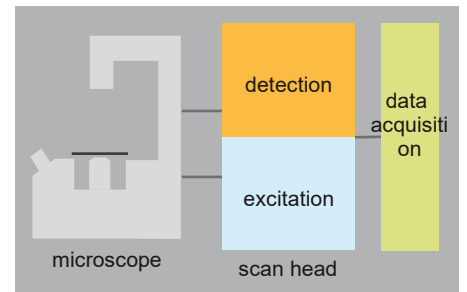

PicoQuant GmbH
 Rudower Chaussee 29 (IGZ)
 12489 Berlin
 Germany

Phone
 Email
 www

+49-30-1208820-0
 info@picoquant.com
 www.picoquant.com

All Information given here is reliable to our best knowledge. However, no responsibility is assumed for possible inaccuracies or omissions. Specifications and external appearances are subject to change without notice. Trademarks or corporate names are used for explanation and identification, to the owner's benefit and without intent to infringe.